

B 9000 SERIES:**INCUBATORS, BACTERIOLOGICAL CABINETS**

Series B9000 consists of four different cabinets ranging in size from 23 litres to 420 litres.

Interior housing and shelves are in stainless steel. All cabinets are equipped with a glass inner door.

Externally, the cabinets are constructed of electrolytically galvanized steel sheets, coated with a grey epoxy polyester paint (RAL 7035).

The three smallest models are table models that are stackable. The largest model is freestanding and has adjustable feet.

**KEY FEATURES**

- ▶ **Automatic safety thermostat** Increased safety – simpler to operate
- ▶ **LCD display** Explanatory text – simpler to operate
- ▶ **Touch buttons** Extended lifetime in humid surroundings
- ▶ **Software** Alternates between two temperatures at specified time, daily or weekly
- ▶ **Extended temperature range** Can operate down to 2°C above ambient temperature
- ▶ **Keypad with PIN code** Prevents undesirable settings
- ▶ **Potential free alarm contact** Can connect to external alarm system
- ▶ **Sterilizing cycle** Possible to sterilize
- ▶ **USB outlet** Simple updates possible via PC
- ▶ **10 speed fan**

TIMERS


In the **System Setup**, one of two timer systems can be chosen:



STANDARD TIMER (DEFAULT):

- Can be set to maximum 99 hours and 59 minutes.
- **Starts counting** down when the **Set Temperature** is reached.
- In the case of power failure, lasting more than 5 minutes, the counting will restart from the beginning.
- The Fan and Air valve (if assembled) are controlled as illustrated below.
- If the chamber shall run without any timing, the time setting should be set to 00h 00m. This will avoid accidental start of the timer.

STANDARD TIMER, EXAMPLE

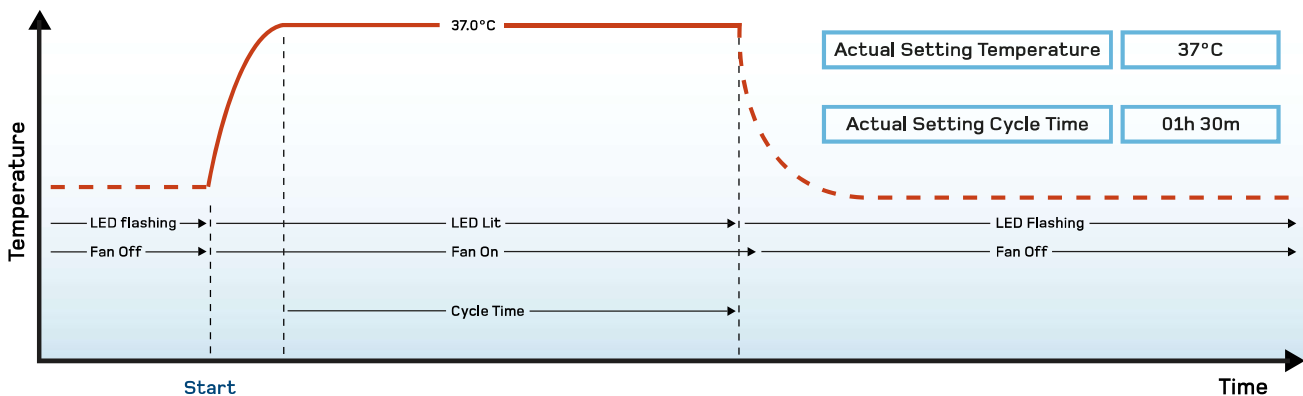


REAL TIME PROGRAM:


- Optional, can be chosen in the System Setup Menu
- Makes it possible to operate the chamber at two different temperatures
- The extra temperature is named **Temperature B** in the menus
- Setting Temperature B to 00.0°C means that heater and fan are turned off in that period. (Sleep Mode)
- **Start- and end Time** for Temperature B can be set to any time during the **week or on daily basis**
- When choosing xx instead of a specified day, the change will occur daily at the given time
- The **Real Time Clock** is backed up for about 10 minutes if power fails. A warning is given if adjustment is needed.



WEEK CYCLE, EXAMPLE

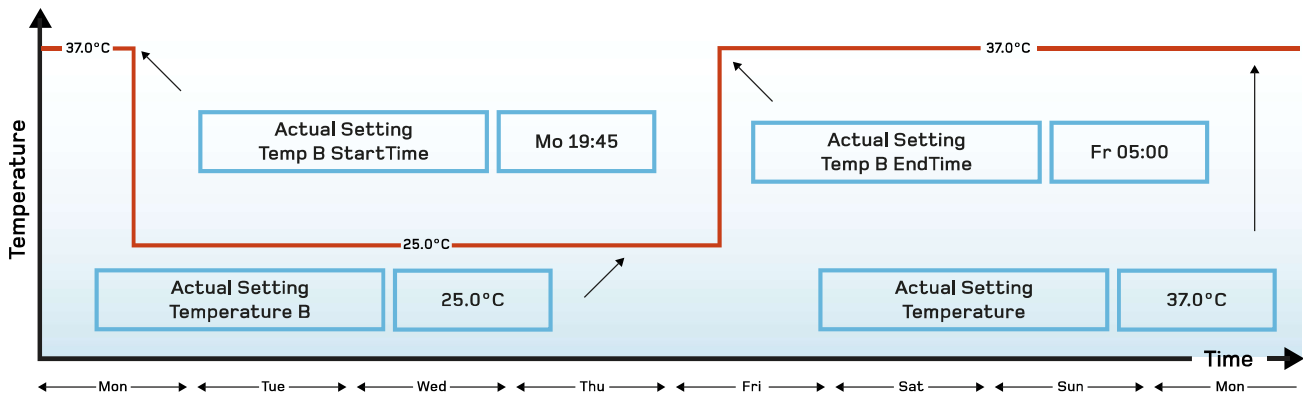

DAY CYCLE, EXAMPLE

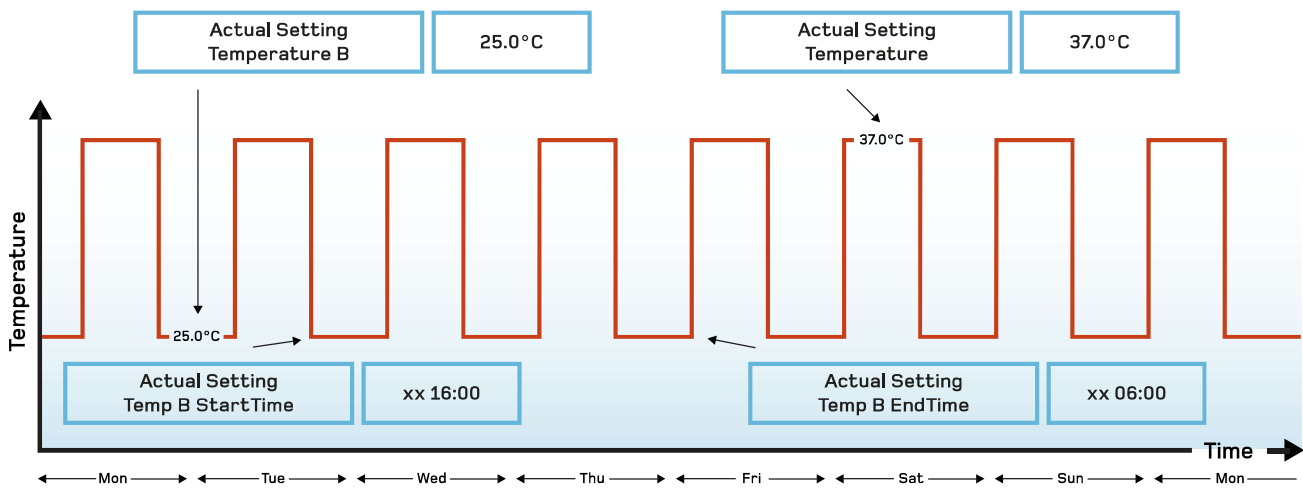

STERILIZATION CYCLE

- A **fixed sterilization cycle** for the chamber is available, 180°C in 40 minutes
- **Standard timer** must have been chosen in the **Setup Menu**
- Acts as Standard Timer, but temperature and time can't be adjusted
- The cycle can be **started** by pressing **Up, Down and Timer keys** for 3 seconds
- The message **Sterilization** appears in the left display and the Timer LED turns on
- **Heating Up** is displayed until the 180°C has been reached
- **Time Left** (Minutes) will be displayed when the set temperature has been reached.
- When finished, **Cycle Complete** will be displayed and the LED starts flashing
- Return to normal operation, timer or continuous, by pressing Timer key for 3 sec

THE FAN

- Adjustable speed, 1 to 10.
- When heating up, settings lower than 6 will be ignored.
- Stops for about 30 seconds when the door is opened while running at set temperature. This function is disabled for 4 minutes after last door opening or after last Air Valve adjustment.
- May reduce speed, or even stop, if operating at a temperature close to the ambient temperature.





PIN CODE

- Optional system to stop unwanted settings from unauthorized persons.
- A **personal pin code** can be entered during the first 30 seconds after turning the chamber on with the main switch or waking up from Standby Mode. Actual code is displayed after pressing the Set key in that period. A unique code can be chosen in the range from 001 to 999.
- 000 means deactivated Pin Code System.
- When activated, **Pin Code?** will be displayed in the left display.
- **Actual code must be set by Up/Down Keys**, followed by pressing the **Enter Key**.
- The system will remain opened for 30 seconds after the last key operation.
- Alarms can be acknowledged by the Standby Key even if the keys are locked.
- If assembled with door lock system, the door will be locked as the keys are locked.

STANDBY

- Preferred way to shut down the chamber. Keeps the real time clock running.
- Turns off Heaters, Fan and Display.
- Press the Standby Key for about 3 seconds until the backlight in the display turns off.
- The Standby LED turns on when the key is released.
- The chamber can be restarted by pressing the Standby Key for 3 seconds.
- The right display will show Wait... for a moment during initialization.

CALIBRATION

Two calibration constants can be adjusted in order to bring the temperature measurement equal to the true value according to a control device.

ALARMS

- A number of alarm situations may occur, listed below.
- Actual warning is given in the lower line of the left display.
- The backlight starts flashing and the buzzer starts sounding whenever an alarm occur.
- The flashing and the sound can be stopped by pressing the Standby Key.

ALARM OUTPUT

- A potential free contact is available for external use (see drawing Main Switch and External Connections).
- The output switches when an alarm situation occurs, one minute delayed.
- Switches immediately at power failure.
- Immediate return to normal when the alarm situation is over.

SAFETY THERMOSTAT

- Automatic system, preventing risky temperatures in the case of a controller failure.
- Completely independent from the ordinary temperature control system.
- Automatically adjusted whenever a new Temperature Set is entered.
- Adjustable limit (offset from target).
- Cuts power to the heaters when the limit is exceeded.
- Generates an alarm warning.
- Turns to normal when the temperature has dropped 0,5°C below the limit.

INCUBATORS, BACTERIOLOGICAL CABINETS

TEMPERATURE CONTROL		B 9025	B 9051	B 9130	B 9420
Variation	+ / - °C	0,2	0,2	0,2	0,2
Deviation (spatial)	+ / - %	1	1	1,5	1,5
Readability / Setability	°C	0,1/0,1	0,1/0,1	0,1/0,1	0,1/0,1
Range	°C	t _b -99,9	t _b -99,9	t _b -99,9	t _b -99,9
Sensor thermocouple "K"		Yes	Yes	Yes	Yes
Controller		PID	PID	PID	PID
Display		LCD	LCD	LCD	LCD

TIMER

Standard hours/minutes		99h/59m	99h/59m	99h/59m	99h/59m
Real time program *		Yes	Yes	Yes	Yes

SAFETY

Alarm flashing / Acoustic		Yes	Yes	Yes	Yes
Alarm limit settable	°C	Yes	Yes	Yes	Yes
Automatic safety setting	°C	Yes	Yes	Yes	Yes

FEATURES

Fan speed steps		1/10	1/10	1/10	1/10
Door gasket silicone		Yes	Yes	Yes	Yes
Glass innerdoor		Yes	Yes	Yes	Yes
Data port, Serial USB		Yes	Yes	Yes	Yes
Pot free alarm, output		Yes	Yes	Yes	Yes

SHELVES

Standard / Max	pcs	2/7	2/8	3/16	3/23
Dimensions WxD	mm	346 x 235	434 x 325	534 x 325	602 x 570
Max load pr shelf	kg	20	20	20	30
Permitted total load	kg	50	50	70	100

HEATING

Heating up time to 37°C	mins	27	30	33	30
Heat transfer at 70°C	W	65	75	90	190

POWER

Nominal Power	W	480	480	930	1430
Nominal voltage	V	230,1~	230,1~	230,1~	230,1~
Frequency	Hz	50/60	50/60	50/60	50/60

DIMENSIONS

Exterior WxDxH	mm	490x480x500	580x575x550	680x675x750	753x845x1360
Interior WxDxH	mm	350x255x300	440x345x350	540x455x555	610x600x1180
Volume	litres	25	51	130	420

WEIGHTS / VOLUME

Net weight	kg	20	35	52	120
Shipping weight	kg	25	40	60	140
Shipping volume	dm ³	0,21	350	558	1280

t_b = 2°C ABOVE AMBIENT

* CAN BE SET AT TWO TEMPERATURES, DAILY OR WEEKLY